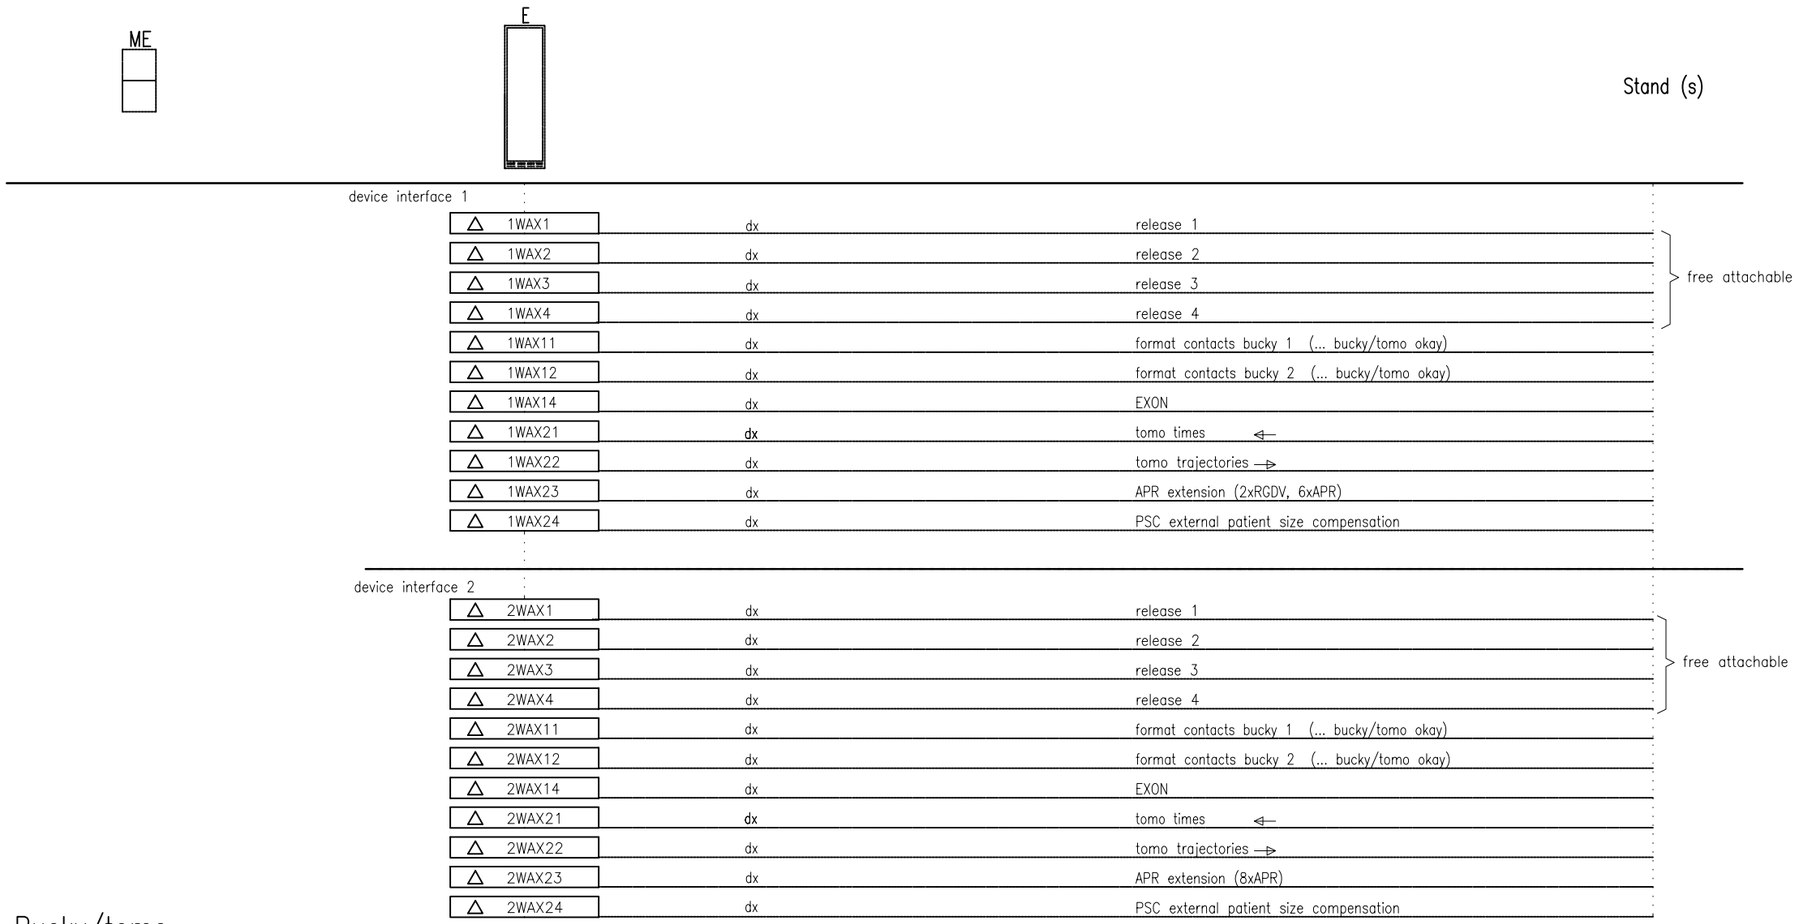
ME
E
Stand (s)
device interface 1
1WAX1 dx release 1
1WAX2 dx release 2
1WAX3 dx release 3
1WAX4 dx release 4
free attachable
1WAX11 dx format contacts bucky 1 (... bucky/tomo okay)
1WAX12 dx format contacts bucky 2 (... bucky/tomo okay)
1WAX14 dx EXON
1WAX21 dx tomo times
1WAX22 dx tomo trajectories
1WAX23 dx APR extension (2xRGDV, 6xAPR)
1WAX24 dx PSC external patient size compensation
device interface 2
2WAX1 dx release 1
2WAX2 dx release 2
2WAX3 dx release 3
2WAX4 dx release 4
free attachable
2WAX11 dx format contacts bucky 1 (... bucky/tomo okay)
2WAX12 dx format contacts bucky 2 (... bucky/tomo okay)
2WAX14 dx EXON
2WAX21 dx tomo times
2WAX22 dx tomo trajectories
2WAX23 dx APR extension (8xAPR)
2WAX24 dx PSC external patient size compensation

Bucky/tomo
for examination units without CAN-interface

A3 01-11-21 Schr./Ost.
4512982009 21_z7_3_010

OPTIMUS RAD
Connection diagram

© Philips Medical Systems